


Vaccine Storage Temperatures



Refrigerator Temperatures

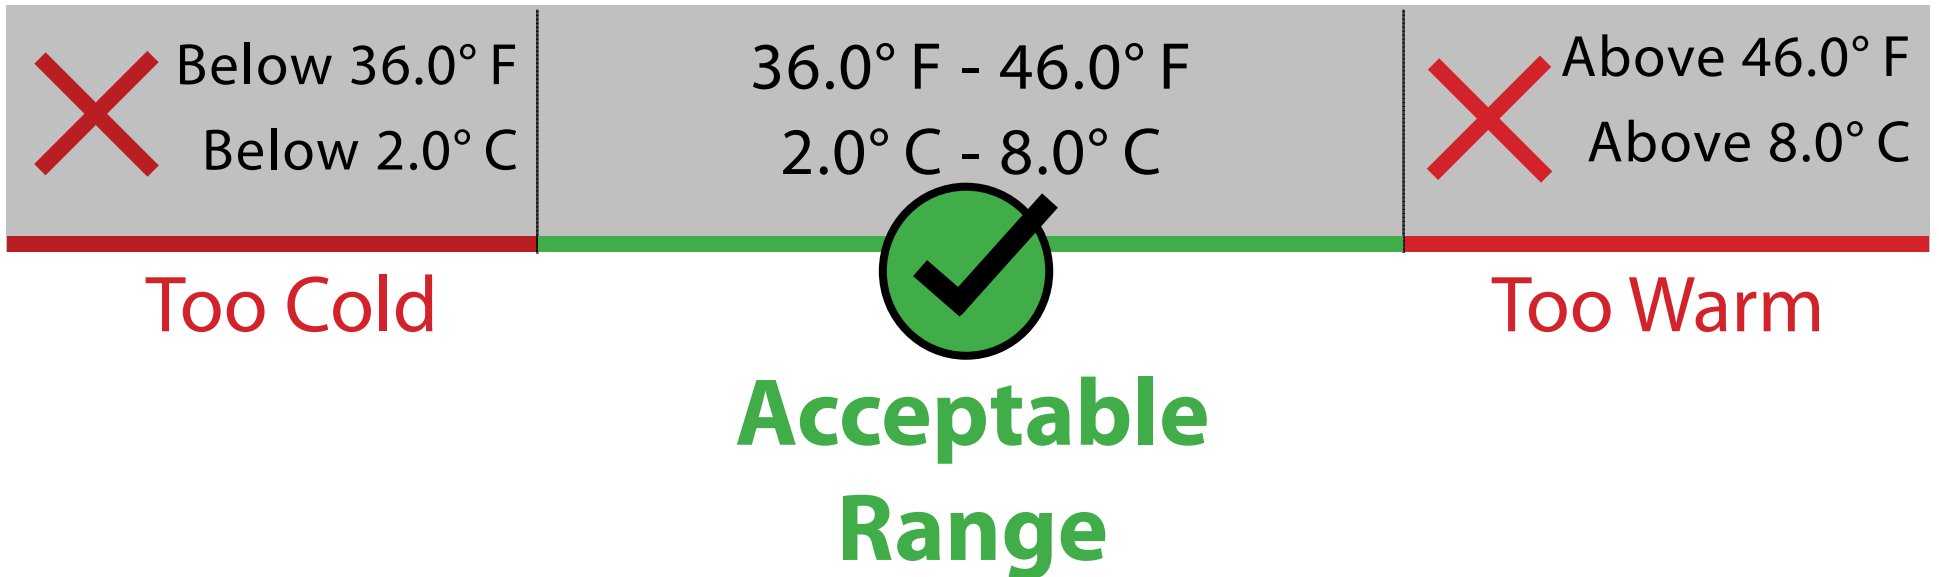

If your DDL indicates an alarm:

- Record the time and temperature.
- Download the DDL file and email it to TempCheck@phila.gov.
- Follow TempCheck's instruction to confirm the viability of the vaccines. Do not use the vaccines in the affected storage unit until the viability has been confirmed.
- If TempCheck tells you to fill out an Emergency Temperature Response Form, fill it out and send it to TempCheck@phila.gov or fax it to 215-238-6948 within 48 hours of the out-of-range temperature.